


# KELRON

[www.kelroninc.com](http://www.kelroninc.com)

## Kelron Duo Leak Check Instructions

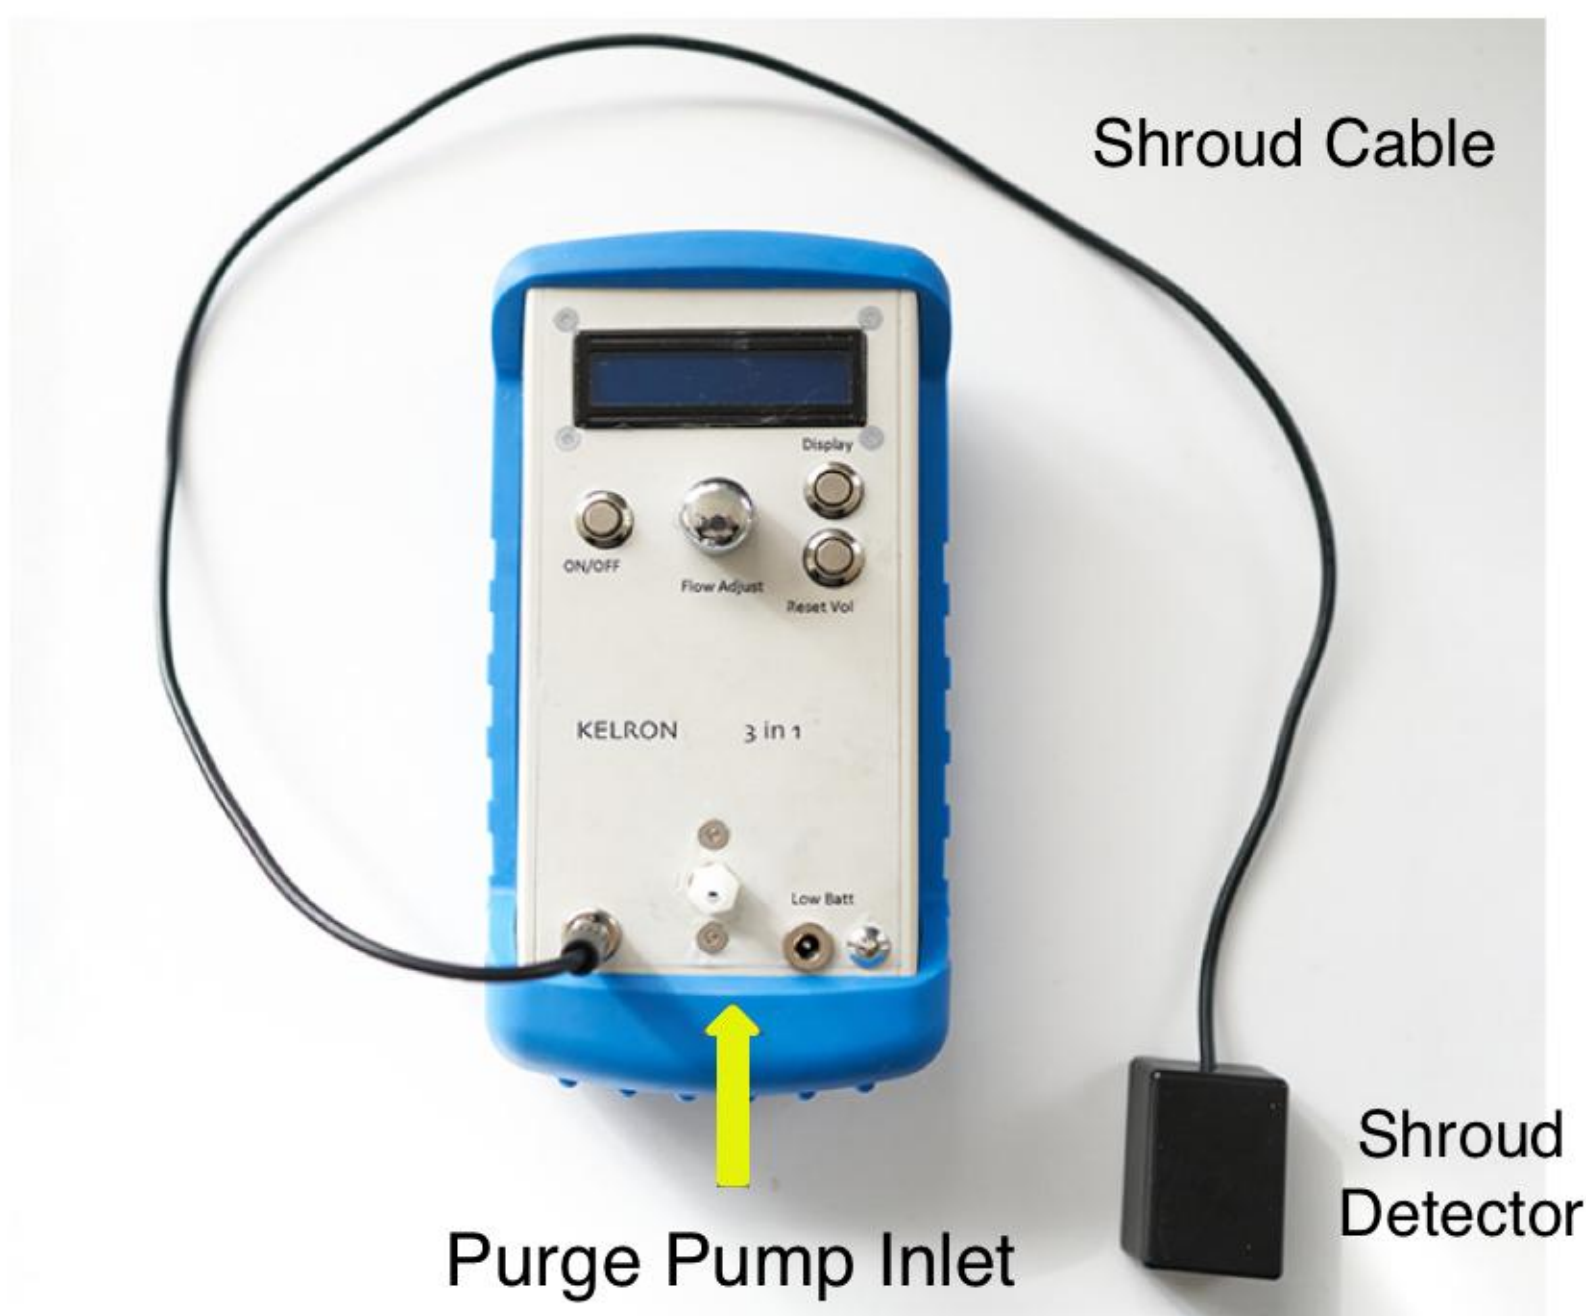

1. Place the shroud detector inside Helium shroud and thread the shroud cable out through port. Plug the shroud detector cable into the unit located outside of the shroud. If multiple Kelrons are in use match the shroud cable and main unit number.
2. Press the power button, unit will display warm-up countdown. Do not expose the unit or shroud detector to helium during the warm-up countdown.
3. Once warm-up is complete, attach purge tubing to the unit.
4. Press Display button to show purge pump flow rate. Press again to return to Helium readings.
5. Turn the flow adjust knob clockwise and adjust flow rate.
6. Total volume purged will appear on the screen. Reset Vol button will zero the volume reading for the next sample.
7. Press the display button again to display Helium concentrations.
8. Proceed to purge and sample per your workplan.
9. Monitor the purge line at all times for moisture, do not allow droplets of water to enter device.



Scan QR Code to provide feedback